

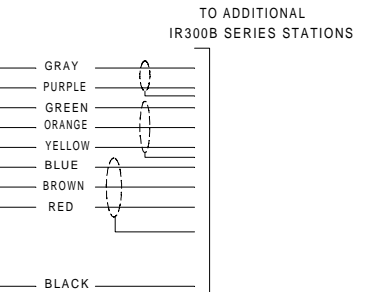


GROUND IN ACCORDANCE  
WITH NEC ARTICLE 250 & 517

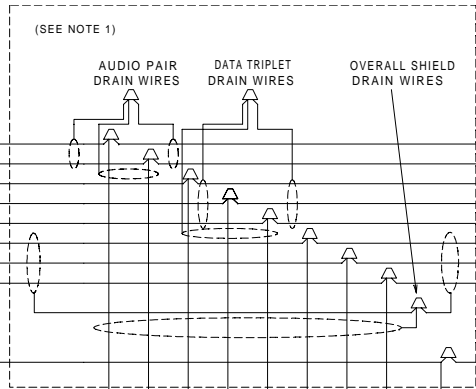

**NOTES:**

1. Shields must be isolated from each other and continuous to splice point to the last station on the port.
2. Shields must be isolated from each other and from any ground.

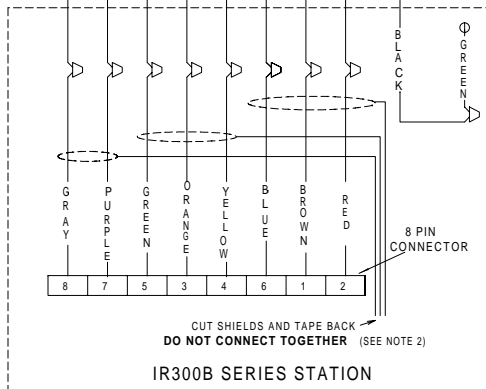

**TekTone®**

TITLE: Connector Circuit Interconnections  
for Addressable Stations  
APP: NC300 NURSE CALL SYSTEM

MATL: MEL  
REV: 5

DATE: 12/23/98  
PAGE: NL410